






MARIA™
Premixed Multiplex Array for Indoor Allergens (5-plex)

Product Code: MRA-P5B

Lot Number: xxxxx

MARIA™ Allergen Assays



www.inbio.com


Indoor Biotechnologies, Inc.
1216 Harris Street,
Charlottesville
Virginia, 22903
United States

Tel: (434) 984-2304
Fax: (434) 984-2709
mail@inbio.com

Indoor Biotechnologies Ltd
The Old Brewery
38, High Street, Warminster
Wiltshire, BA12 9AF
United Kingdom

Tel: 44 (0)5601 153 291
Fax: 44 (0)1985 218 300
info@indoorbiotech.co.uk

**Storage: The MARIA™ kit should be stored at 4°C
(QC samples and UAS should be frozen following receipt)**

INDOOR and  are Registered Trademarks of INDOOR biotechnologies, Ltd.,
Manchester U.K.

For Research Use Only: Not for Diagnostic or Therapeutic Use

7. Assay Performance

| | MARIA™ | | | |
|----------------|-----------|-----------------|-----------------|----------------------------|
| | mAb Pairs | Intra-Assay %CV | Inter-Assay %CV | Limit of Detection (ng/mL) |
| Der p 1 | 10B9/5H8 | 4.4 | 7.3 | 0.06 |
| Der f 1 | 6A8/4C1 | 5.0 | 5.4 | 0.06 |
| Fel d 1 | 6F9/3E4 | 4.0 | 5.3 | 0.02 |
| Can f 1 | 10D4/6E9 | 4.3 | 11.8 | 0.06 |
| Bla g 2 | 1F3/4C3 | 3.3 | 5.4 | 0.98 |

8. Materials Required but Not Provided






A. Reagents

1. Assay buffer. Buffer recipes can be found on our web site: www.inbio.com/MARIA.html
2. Luminex Sheath Fluid (Luminex Catalog #40-50000, BioRad Catalog# 171000055)

B. Instrumentation/Materials

1. Adjustable Pipettes with Tips (10 µl - 1000 µl)
2. Multichannel Pipettes (5 µl - 50 µl and 25 µl - 200 µl)
3. Reagent Reservoirs
4. Polypropylene Microcentrifuge Tubes
5. Aluminum Foil or Drawer (incubation in dark)
6. Absorbent Pads or Paper Towels
7. Laboratory Vortex
8. Vacuum Filtration Unit (Millipore Vacuum Manifold, Catalog # MAVM0960R)
9. Luminex xMAP® Instrument

6. Sample Curves

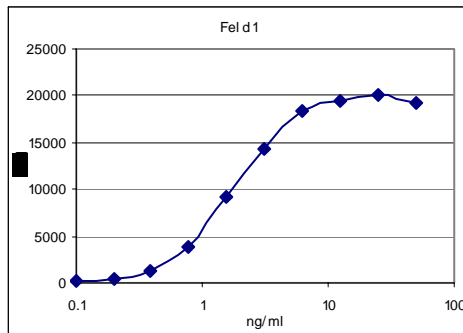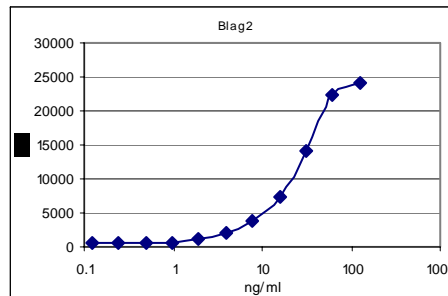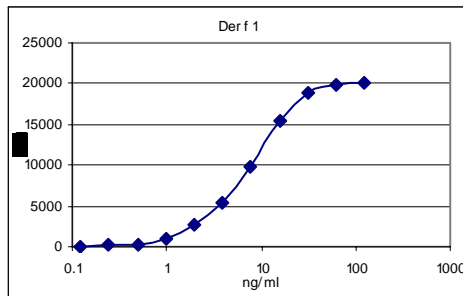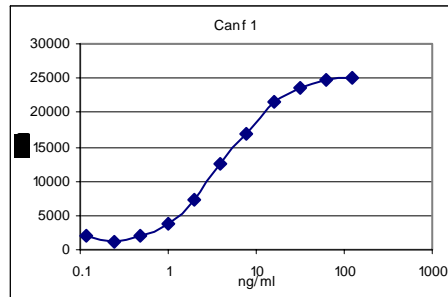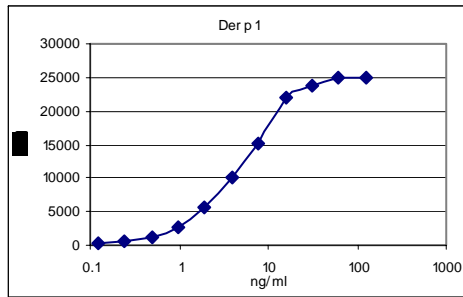

MARIA™ Premixed Multiplex Array for Indoor Allergens

1. Intended use
2. Reagents supplied
3. Assay Workflow
4. Certificate of Analysis
5. MARIA™ Protocol
6. Sample Curves
7. Assay Performance
8. Materials Required but Not Provided

By opening the packaging containing this Kit (which contains fluorescently labeled microsphere beads authorized by Luminex Corporation) or using this Kit in any manner, you are consenting and agreeing to be bound by the following terms and conditions. You are also agreeing that the following terms and conditions constitute a legally valid and binding contract that is enforceable against you. If you do not agree to all of the terms and conditions set forth below, you must promptly return this Kit for a full refund prior to using it in any manner.

You, the customer, acquire the right under Luminex Corporation's patent rights, if any, to use this Kit or any portion of this Kit, including without limitation the microsphere beads contained herein, only with Luminex Corporation's laser based fluorescent analytical test instrumentation marketed under the name Luminex Instrument. The Luminex Instrument refers to Luminex® 100, Luminex 200 and other Luminex Instruments available from Luminex Corporation and from authorized distributors including Bio-Rad Laboratories (Hercules, CA), Qiagen Corporation (Valencia, CA) and MiraiBio (South San Francisco, CA).

5. MARIA Protocol (cont.)

1. INTENDED USE

This is a multiplex assay kit manufactured by INDOOR Biotechnologies Inc. to be used for the simultaneous quantitative determination of five common indoor allergens: house dust mite allergens Der p 1 (*Dermatophagoides pteronyssinus*) and Der f 1 (*Dermatophagoides farinae*) and animal allergens Fel d 1 (cat, *Felis domesticus*), Can f 1 (dog, *Canis familiaris*) and Bla g 2 (cockroach, *Blattella germanica*).

This kit may be used for analysis of the above indoor allergens in environmental samples, such as house dust extracts or air filter samples and other biologic or environmental samples.

2. REAGENTS SUPPLIED

- Vial 1 (blue top) 75 µL
Product Code: MS-P5B
Premixed 5-plex Antibody-coupled Fluorescent Microspheres
- Vial 2 (yellow top) 50 µL
Product Code: ST-UAS
Universal Allergen Standard
- Vial 3 (brown top) 100 µL
Product Code: BI-MRA-P5B
Premixed Biotinylated Detector Monoclonal Antibodies (mAb)
- Vial 4 (pink top) 50 µL
Product Code: SAP-MRA
Streptavidin-Phycoerythrin
- Vial 5&6 (purple top) 50 µL
Product Code: QC-MRA
Quality Control Samples: High/Low
- Microtiter Filter Plate
Product Code: FP-MRA
Millipore MultiScreen BV
Millipore catalog # MABVN1250

6. Remove buffer from the 96 well filter plate by vacuum filtration. Tap the plate on paper towels to remove excess buffer from the plate bottom. Repeat vacuum filtration. Tap plate again on paper towels. ***Do Not Invert Plate***

The Assay

7. Pour the microsphere solution into a pipette basin and use a multichannel pipette to add 50 µL of microsphere solution to each well.

- Add 50 µL of diluted standard to duplicate standard wells.
- Add 50 µL of sample dilutions to appropriate wells.
- Add 50 µL of assay buffer to the blank wells.

Set a multichannel pipette to 50 µL and mix all wells vigorously (5-10 repetitions).*

**Note: foaming may occur when mixing*

- Incubate for one hour at room temperature in the dark.

8. Dilute the Biotinylated Detector mAb Mix (Product Code: BI-MRA-P5B) stock solution by adding 100 µL to 12 mL assay buffer.

- Remove samples and standards by vacuum filtration and filter-wash wells 2x with 100 µL assay buffer.*
- Add 100 µL diluted 5-plex Biotinylated Detector mAb Mix to each well and mix vigorously by pipetting.
- Incubate for one hour at room temperature in the dark.

**Note: filter-wash wells by adding 100 µL assay buffer then remove buffer by vacuum filtration. No mixing required*

9. Dilute Streptavidin-Phycoerythrin (Product Code: SAP-MRA) by adding 50 µL to 12mL in assay buffer.

- Remove biotinylated antibody solution by vacuum filtration and filter-wash wells 2x with 100 µL assay buffer. Add 100 µL diluted Streptavidin-Phycoerythrin and mix vigorously by pipetting.
- Incubate for 30 minutes at room temperature in the dark.*

**During this incubation period, prepare the instrument for plate reading according to the manufacturer's instructions.*

10. Remove Streptavidin-Phycoerythrin solution by vacuum filtration and filter-wash wells 2x with 100 µL of assay buffer. Add 100 µL of assay buffer to all wells and resuspend the microspheres by pipetting repeatedly, taking care **not** to create a foam.

11. Wipe the bottom of the filter plate with a paper towel and read the plate on the xMAP Instrument.

5. MARIA Protocol

1. Remove dust samples for analysis from freezer and allow to thaw.
2. Pre-wet each well of the 96 well filter plate with 100 μ L of assay buffer (sterile filtered 1% BSA-PBS-0.02% Tween 20, pH 7.4).

**Tip: When pipetting into the 96 well filter plate, insert the pipette tip at an angle into the bottom corner of the well. This will help ensure that the tip does not puncture the filter.*

Preparation of Microsphere Solution

3. Prepare the microsphere solution by first vortexing the 5-plex Microsphere Mix (Product Code: MS-P5B) for one minute and then adding 75 μ L of the bead mix to a total of 5.5 mL of assay buffer. Mix by vortexing.

The bead set assignments are as follows:

| Analyte | Bead Region |
|---------|-------------|
| Der p 1 | 33 |
| Der f 1 | 51 |
| Fel d 1 | 58 |
| Can f 1 | 20 |
| Bla g 2 | 47 |

Preparation of Standards

4. Prepare a standard curve using doubling dilutions of the Universal Allergen Standard (Product Code: ST-UAS) starting at 1/20: Pipette 15 μ L allergen standard into 285 μ L assay buffer into tube 1, mix well. Transfer 150 μ L from tube 1 to 150 μ L assay buffer in tube 2. Continue to make a total of 12 serial dilutions.

** Tip: To ensure accuracy, it is important to mix reagents containing glycerol thoroughly before and during dilutions**

The standard curve dilutions are from :


- 125-0.06 ng/mL for Der p 1, Der f 1, Can f 1 and Bla g 2.
- 50-0.02 ng/mL for Fel d 1.

Preparation of Samples

5. Vortex samples vigorously for 30 seconds and then centrifuge at 14,000 rpm (16,000 x g) for two minutes. We recommended the following serial dilutions in assay buffer:

- Quality Control Samples (Product Code: QC-MRA) (optional): undiluted
- House dust extracts: 1/10, 1/100 and 1/10,000
- Air filter extracts: undiluted, 1/5 and 1/20.

3. Assay Workflow

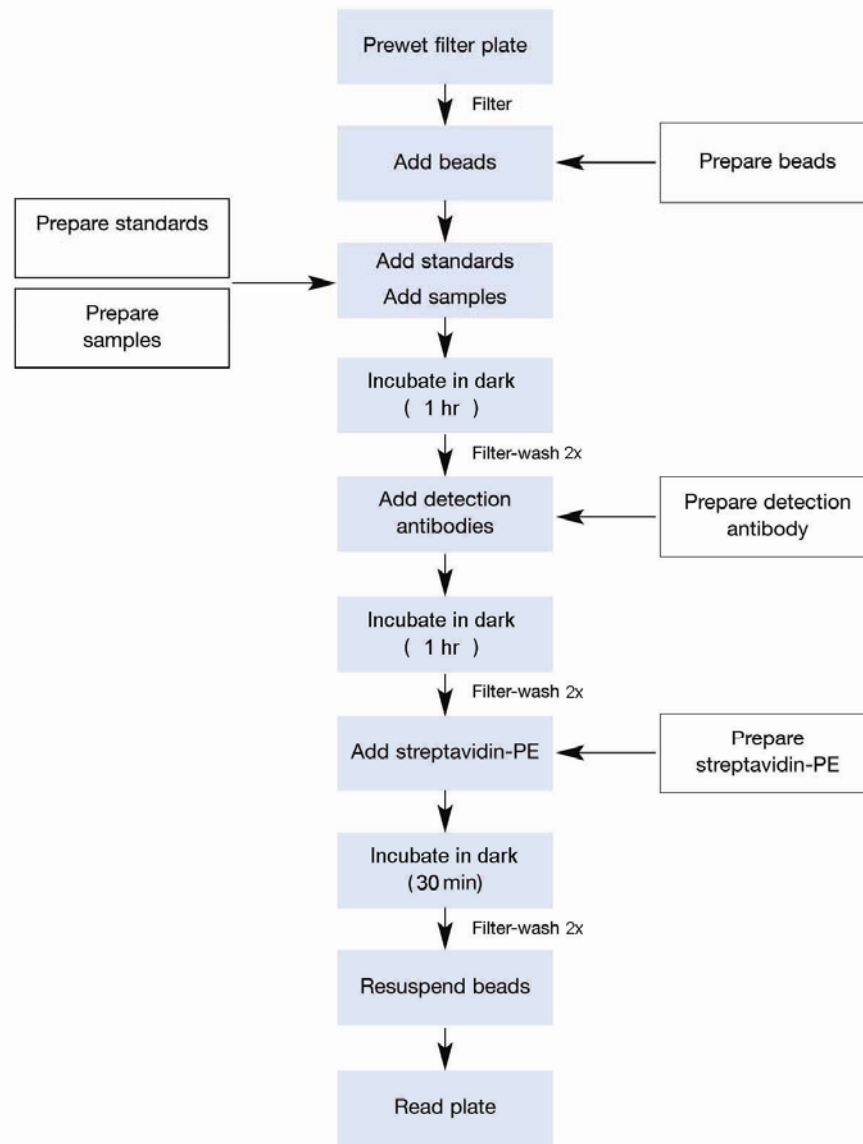

Estimated Assay Time Required:

Sample Preparation: 1 hour; Incubation: 2.5 hours; Plate Reading: 1 hour

4. Certificate of Analysis

Microspheres: Premixed 5-plex Antibody-coupled Fluorescent Microspheres
 Product Code: MS-P5B
 Specificity: mAb against Der p 1, Der f 1, Fel d 1, Can f 1, and Bla g 2

The following microspheres are premixed in the vial provided:

| Analyte | Bead Region | mAb |
|---------|-------------|------|
| Der p 1 | 33 | 10B9 |
| Der f 1 | 51 | 6A8 |
| Fel d 1 | 58 | 6F9 |
| Can f 1 | 20 | 10D4 |
| Bla g 2 | 47 | 1F3 |

Lot Number: xxxxx

Allergen Standard: Universal Allergen Standard
 Product Code: ST-UAS
 Composition: A formulation of eight purified natural allergens prepared in 1% BSA/50% glycerol/PBS, pH 7.4. Keep frozen.

Concentration/Calibration:

| Universal Allergen Standard | Protein Measurement | Concentration (ng/ml) |
|-----------------------------|---------------------|-----------------------|
| Der p 1 | Amino-acid analysis | 2500 |
| Der f 1 | Amino-acid analysis | 2500 |
| Der p 2 | Amino-acid analysis | 1000 |
| Fel d 1 | Amino-acid analysis | 1000 |
| Can f 1 | Amino-acid analysis | 2500 |
| Mus m 1 | Amino-acid analysis | 250 |
| Rat n 1 | Amino-acid analysis | 1000 |
| Bla g 2 | Amino-acid analysis | 2500 |

Lot Number: xxxxx

4. Certificate of Analysis (cont.)

Detector Antibody: Premixed 5-plex Biotinylated Detector mAb
 Product Code: BI-MRA-P5B
 Biotinylation: Biotinylated using EZ-Link Sulfo-NHS-LC Biotinylating Agent and titrated for use in the array.
 Prepared in 1% BSA/50% glycerol/PBS, 0.22µm filtered, preservative free.

The following biotinylated mAb are premixed in the vial provided:

| Analyte | mAb |
|---------|-----|
| Der p 1 | 5H8 |
| Der f 1 | 4C1 |
| Fel d 1 | 3E4 |
| Can f 1 | 6E9 |
| Bla g 2 | 4C3 |

Lot Number: xxxxx

Quality Control Samples: High/Low
 Product Code: QC-MRA
 Composition: A formulation of high/low positive controls prepared in PBS-T 0.02%, 1% BSA, pH 7.4. Keep frozen.

Concentration/Calibration:

| | High QC Sample | | | Low QC Sample | | |
|---------|------------------|------|------|------------------|------|------|
| | Expected (ng/ml) | -30% | +30% | Expected (ng/ml) | -30% | +30% |
| Der p 1 | 8.3 | 5.8 | 10.8 | 1.67 | 1.2 | 2.2 |
| Der f 1 | 8.3 | 5.8 | 10.8 | 1.67 | 1.2 | 2.2 |
| Fel d 1 | 3.3 | 2.3 | 4.3 | 0.67 | 0.5 | 0.9 |
| Can f 1 | 8.3 | 5.8 | 10.8 | 1.67 | 1.2 | 2.2 |
| Bla g 2 | 8.3 | 5.8 | 10.8 | 1.67 | 1.2 | 2.2 |

Lot Number: xxxxx, xxxxx